



# カタログファイルのインポート および管理方法

株式会社ベリタス

2023/9/8



# カタログファイル名のルールとファイルの更新

試薬例	カタログファイル名
マイクロSSP JPN Lot007	SSPJPN_007_16.cat 「製品コード_製品ロット_バージョン」
LABType XR B locus Lot004	RSSOX1B_004_06.cat 「製品コード_製品ロット_バージョン」
LABScreen Single Antigen Class I Lot010 + LS-NC Lot018	LS1A04_NC018_010_01.cat 「製品コード_NC血清のロット_製品ロット_バージョン」
LABScreen Single Antigen Class I Lot010 + C1qScreen Lot012 + C1qNC血清 Lot005	LS1A04CQ12NS5_010_00.cat 「製品コード、C1qのロット、C1q用NC血清のロット_製品ロット_バージョン」

- One Lambdaで行われるカタログファイルの更新タイミング
  - タイピング試薬：血清型ファイルの更新時 + ビーズ情報に変更があった時
  - 抗体検査試薬：ビーズ情報に変更があった時
  - 更新されるとバージョンの数字が増加
- 解析時は必ず最新のカタログファイルを使用してください

# HLA Fusionへのカタログファイルインポート①

- Utilities>Update Reference>Update Reference Fileの順にクリック

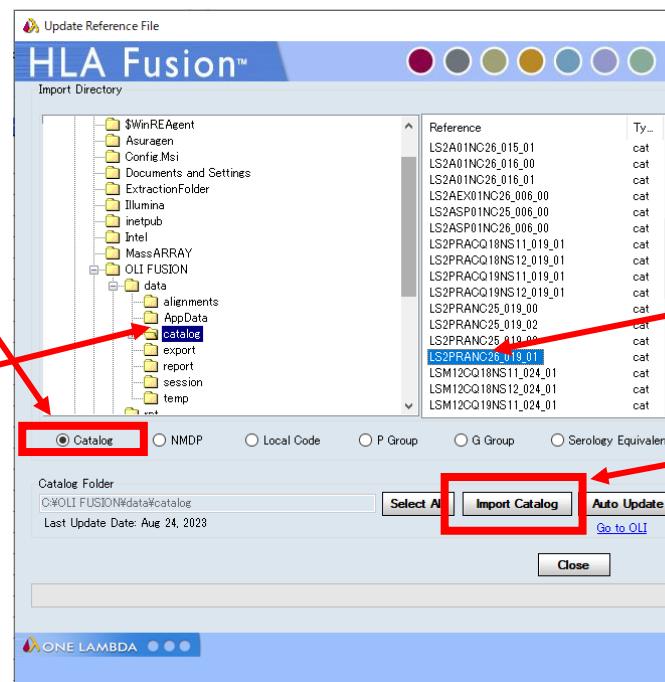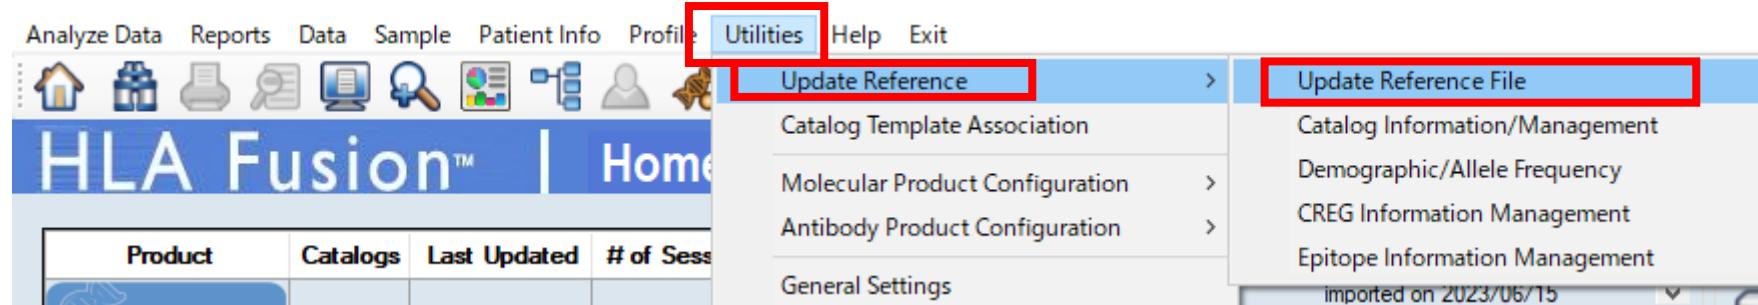

①「Catalog」を選択

②カタログファイルを保存した  
フォルダを選択



③インポートする  
カタログファイルを選択

④「Import Catalog」をクリック

# HLA Fusionへのカタログファイルインポート②

⑤選択したカタログファイルが  
1番左に表示されていることを確認

⑥「Close」をクリック

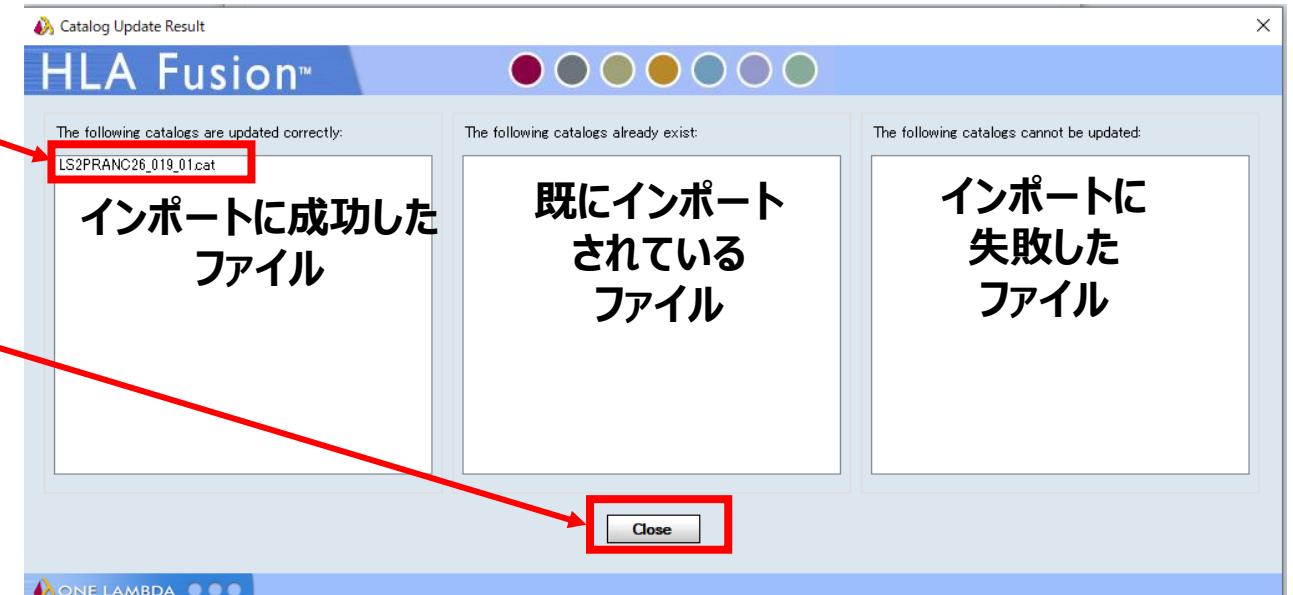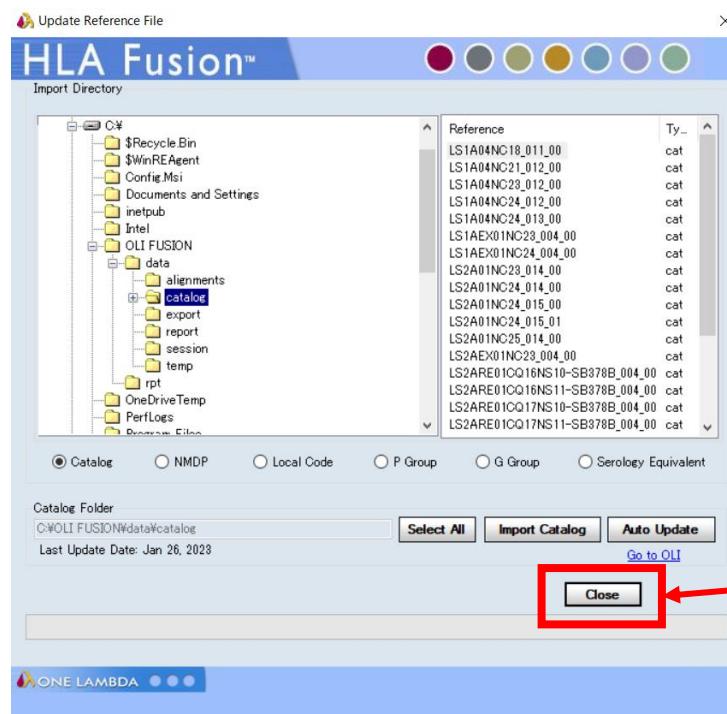

⑦「Close」をクリック

# カタログファイルの管理：利用可能なファイルのリスト



- Homeボタンを押してリストを更新

The screenshot shows the HLA Fusion software interface. On the left, there is a toolbar with various icons: Analyze Data, Reports, Data, Home, and others. The 'Home' icon is circled in red. A yellow arrow points from this icon to the main window. The main window title is 'HLA Fusion™ | Home'. It displays a table of products and their details:


Product	Catalogs	Last Updated	# of Sessions	# of Tests	Recent Session
LABType	6	2023/07/17	13	40	2023/08/22
SSP	3	2023/05/23	1	1	2023/05/23
LABScreen	19	2023/09/01	11	43	2023/08/24

Below this, there is a section titled 'System' with system information and a 'Data and Catalogs' section with download, printer, and catalog options. The bottom half of the screen shows a large table titled 'Product Documents' containing a list of catalog entries. One entry, 'LS2PRANC26\_019\_01', is highlighted with a red box.

インポートしたカタログファイルの一覧  
※アーカイブしたファイルは表示されません

# カタログファイルの管理：非表示（アーカイブ）方法①

- Home画面の「Catalog」ボタンをクリック

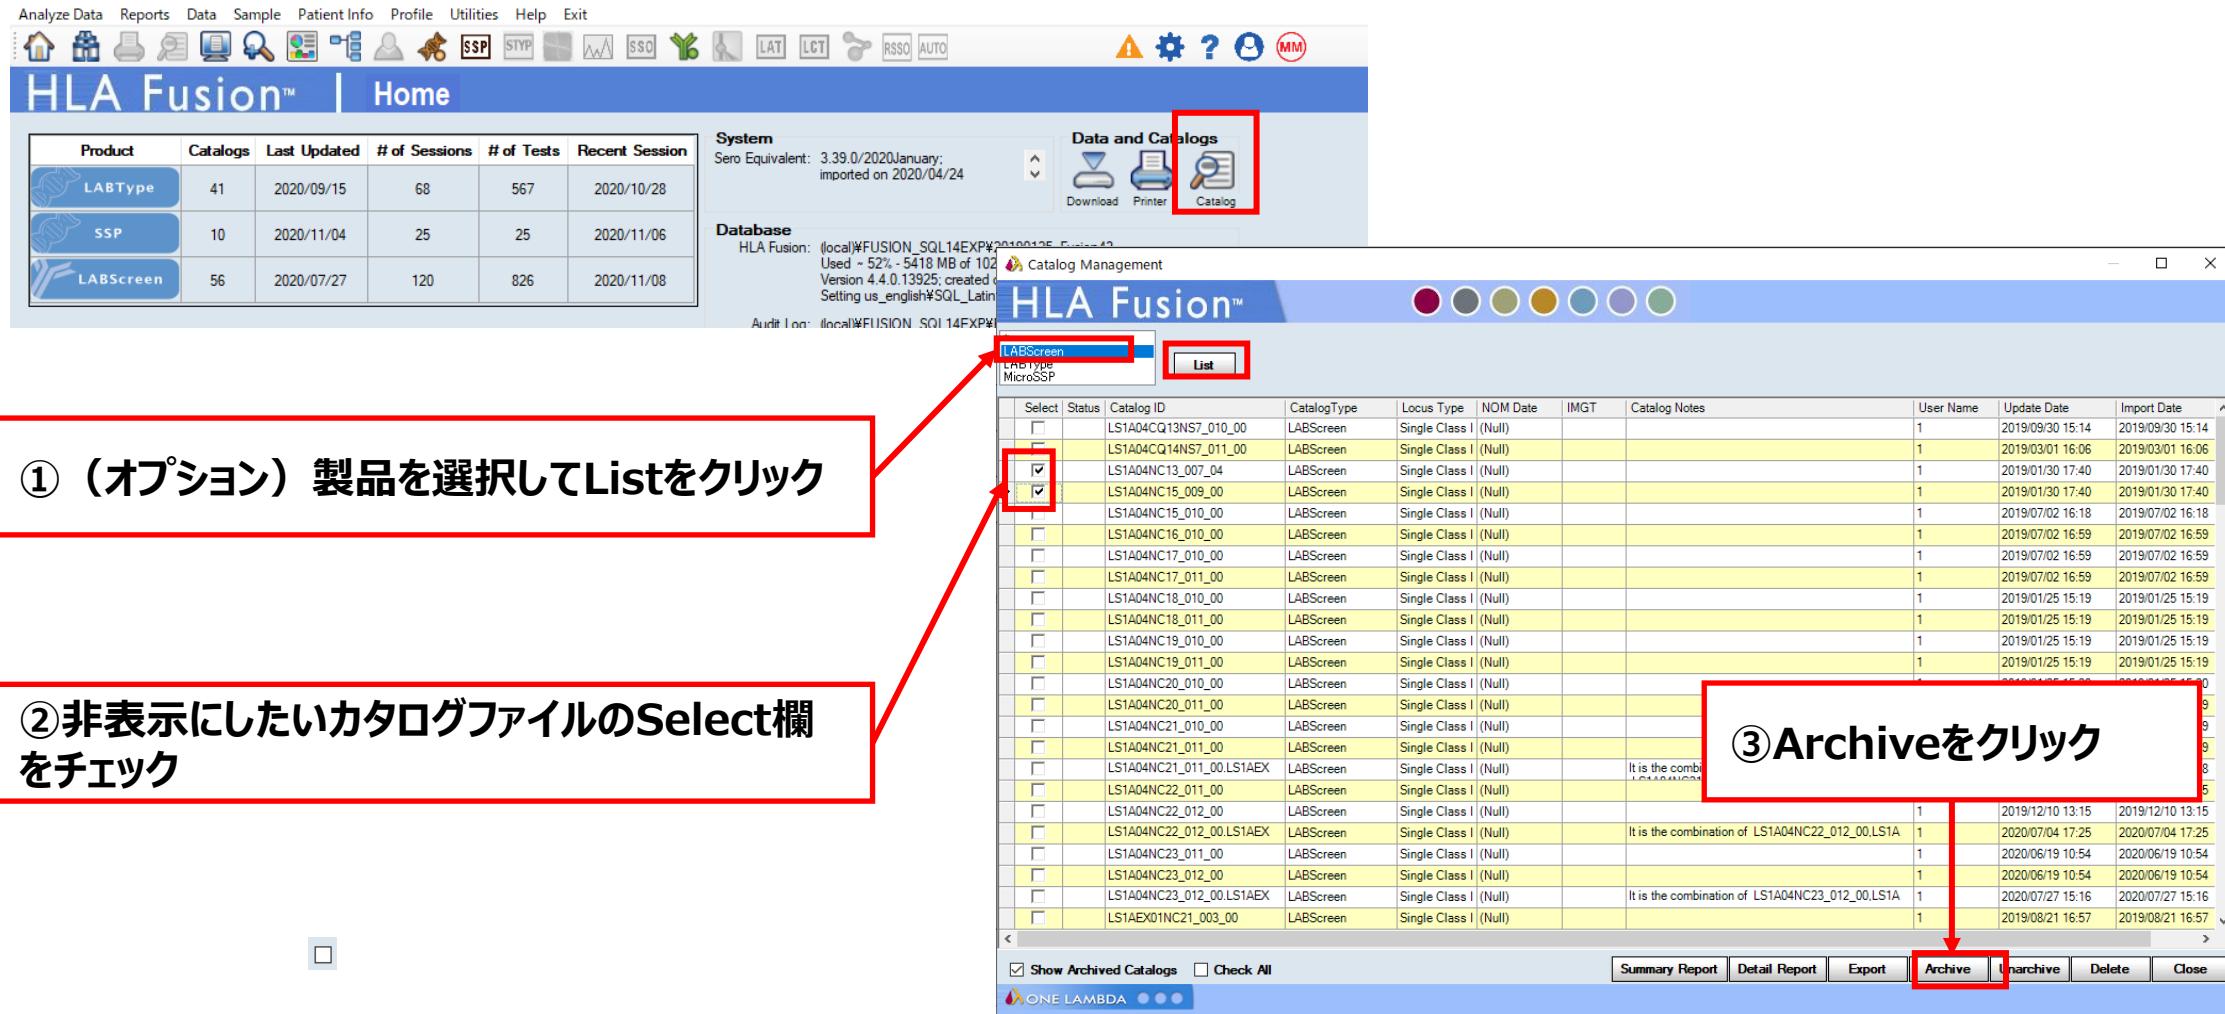


① (オプション) 製品を選択してListをクリック

② 非表示にしたいカタログファイルのSelect欄をチェック

③ Archiveをクリック

Analyze Data Reports Data Sample Patient Info Profile Utilities Help Exit  
HLA Fusion™ Home  
Product Catalogs Last Updated # of Sessions # of Tests Recent Session  
LABType 41 2020/09/15 68 567 2020/10/28  
SSP 10 2020/11/04 25 25 2020/11/06  
LABScreen 56 2020/07/27 120 826 2020/11/08  
System Sero Equivalent: 3.39.0/2020January; Imported on 2020/04/24  
Database HLA Fusion: (local)\FUSION\_SQL14EXPY...  
Audit Log: local\FUSION\_SQL14EXPY...  
Data and Catalogs Download Printer Catalog  
Catalog Management HLA Fusion™  
LABScreen List  
Select Status Catalog ID CatalogType Locus Type NOM Date IMGT Catalog Notes User Name Update Date Import Date  
LS1A04CQ13NS7\_010\_00 LABScreen Single Class I (Null)  
LS1A04CQ14NS7\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC13\_007\_04 LABScreen Single Class I (Null)  
LS1A04NC15\_009\_00 LABScreen Single Class I (Null)  
LS1A04NC15\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC16\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC17\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC17\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC18\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC18\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC19\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC19\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC20\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC20\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC21\_010\_00 LABScreen Single Class I (Null)  
LS1A04NC21\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC21\_011\_00.LS1AEX LABScreen Single Class I (Null)  
LS1A04NC22\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC22\_012\_00 LABScreen Single Class I (Null)  
LS1A04NC22\_012\_00.LS1AEX LABScreen Single Class I (Null)  
LS1A04NC23\_011\_00 LABScreen Single Class I (Null)  
LS1A04NC23\_012\_00 LABScreen Single Class I (Null)  
LS1A04NC23\_012\_00.LS1AEX LABScreen Single Class I (Null)  
LS1AEX01NC21\_003\_00 LABScreen Single Class I (Null)  
Show Archived Catalogs Check All Summary Report Detail Report Export Archive Delete Close  
ONE LAMBDA

# カタログファイルの管理：非表示（アーカイブ）方法②

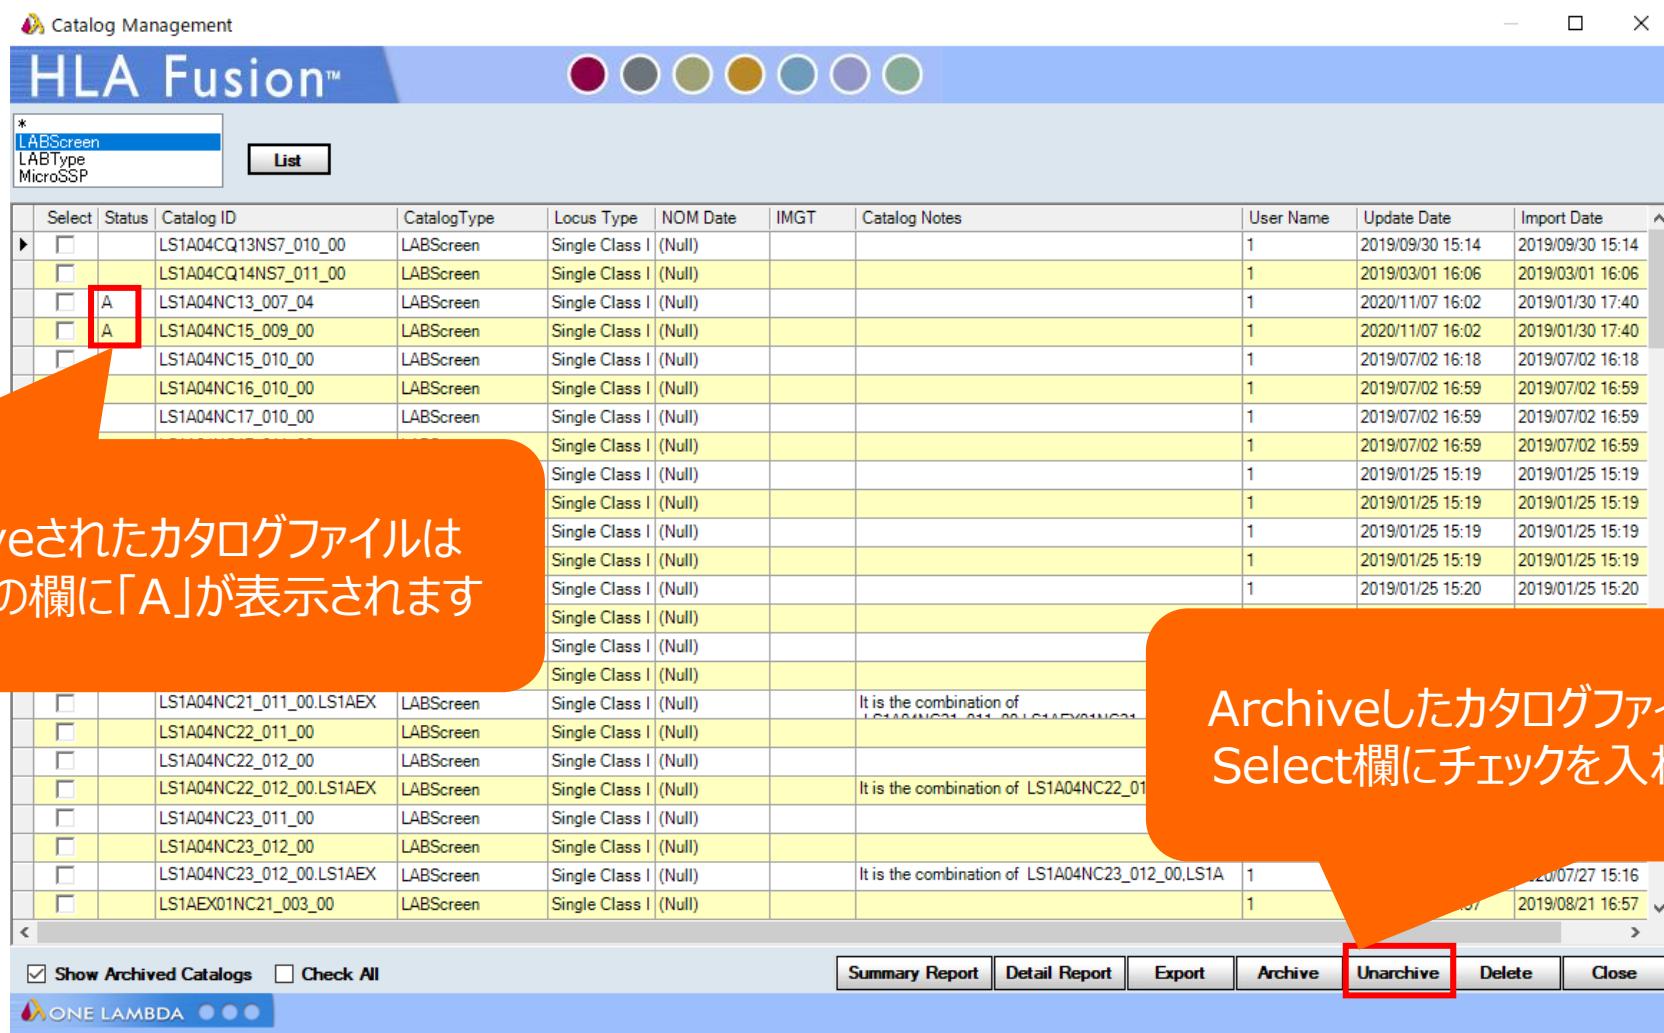


The screenshot shows the HLA Fusion Catalog Management interface. At the top, there's a navigation bar with tabs like 'Catalog Management' and 'HLA Fusion™'. Below it is a search bar with fields for 'Catalog ID' (containing 'LABScreen'), 'LABType' (containing 'MicroSSP'), and a 'List' button. The main area is a grid of catalog entries. The first two rows are highlighted in yellow. The third row has a red box around its 'Status' cell, which contains the letter 'A'. The fourth row also has a red box around its 'Status' cell, which also contains 'A'. The grid columns include 'Select', 'Status', 'Catalog ID', 'CatalogType', 'Locus Type', 'NOM Date', 'IMGT', 'Catalog Notes', 'User Name', 'Update Date', and 'Import Date'. In the bottom right corner of the grid, there's a note: 'It is the combination of LS1A04NC21\_011\_00,LS1AEX01NC21\_003\_00'. At the bottom of the screen, there's a toolbar with buttons for 'Summary Report', 'Detail Report', 'Export', 'Archive' (which is highlighted with a red box), 'Unarchive' (also highlighted with a red box), 'Delete', and 'Close'. There are also checkboxes for 'Show Archived Catalogs' and 'Check All'. The footer of the application includes the 'ONE LAMBDA' logo.

Archiveされたカタログファイルは  
Statusの欄に「A」が表示されます

Archiveしたカタログファイルを再表示する場合は  
Select欄にチェックを入れ、Unarchiveをクリック

# アーカイブ前後の例

- LABScreen Mixed Lot023/024 + NC血清ロット25/26以外をArchive

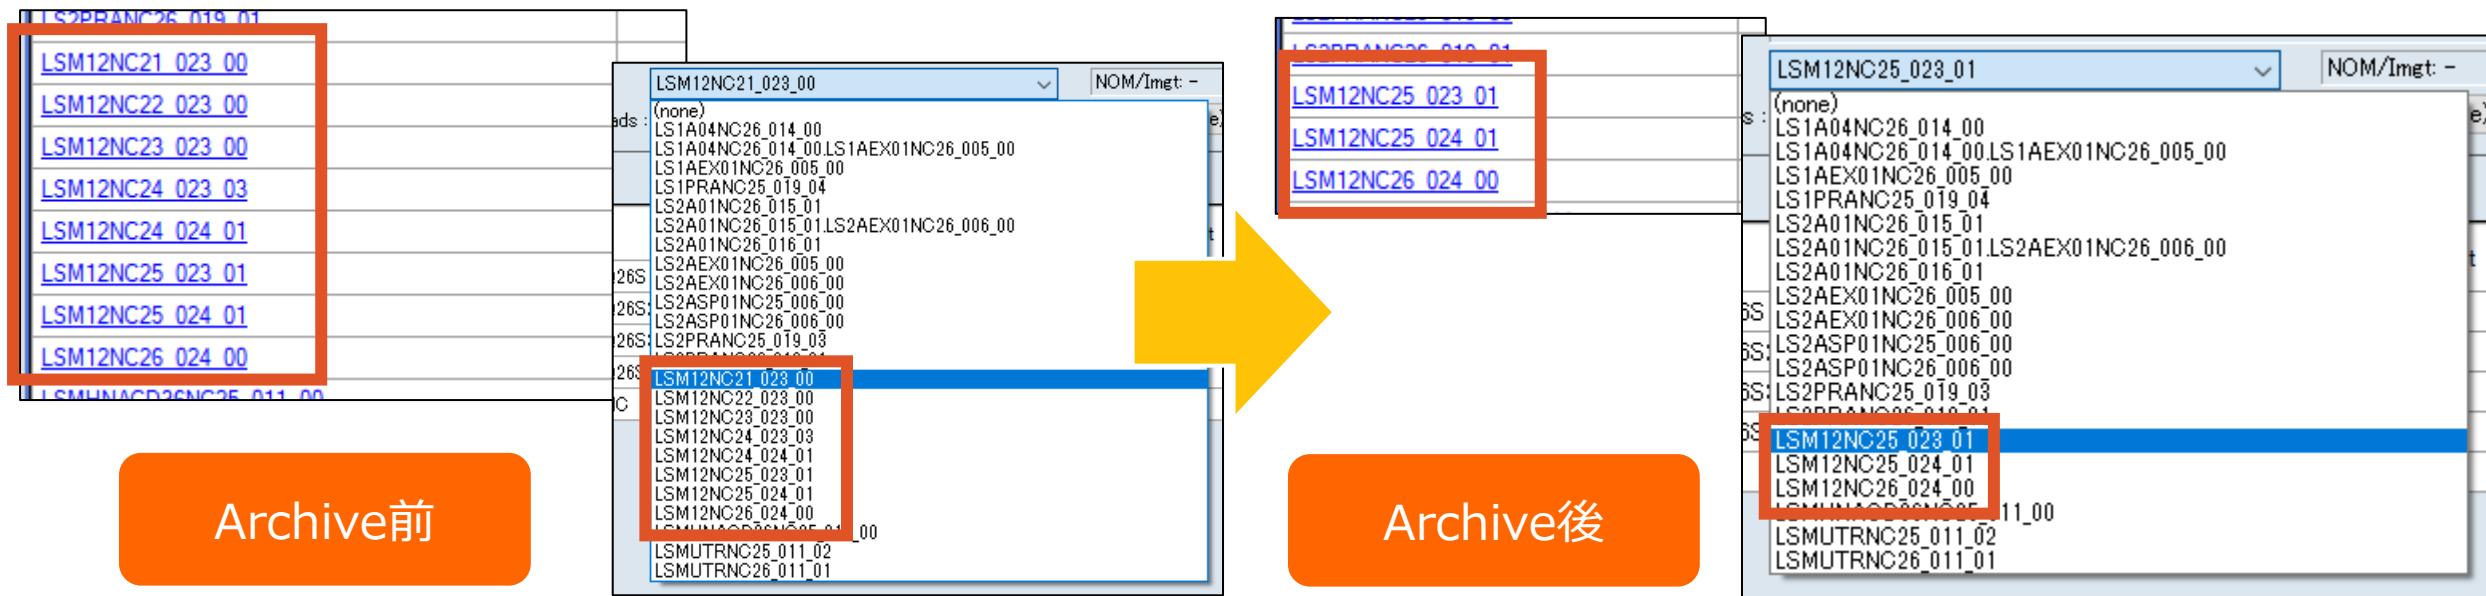

- アーカイブしたカタログファイルはデータ解析のカタログリストやHome画面に表示されません
- NC血清のロットや試薬ロットが変更になった場合は、旧ロットのカタログファイルをアーカイブすることをおすすめします